



## SYSTEMS AND METHODS FOR DEPLOYING A BIOSENSOR WITH A STENT GRAFT Lone Wolinsky, et al 09/522,724



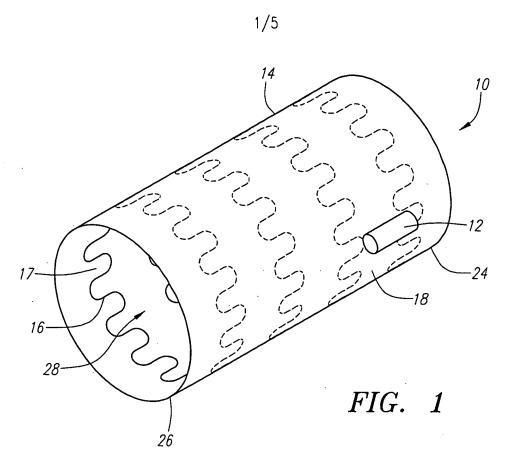

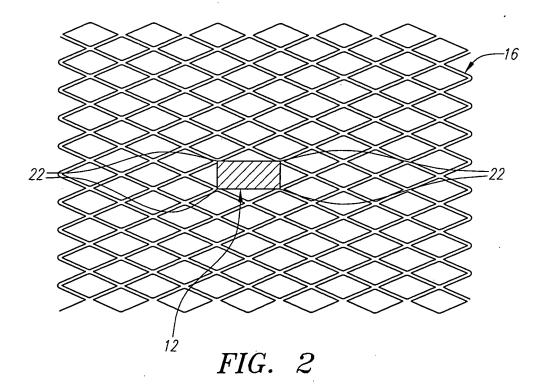

2/5

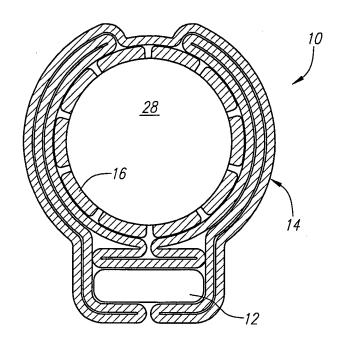


FIG. 3A

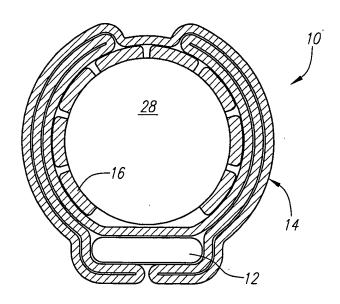


FIG. 3B



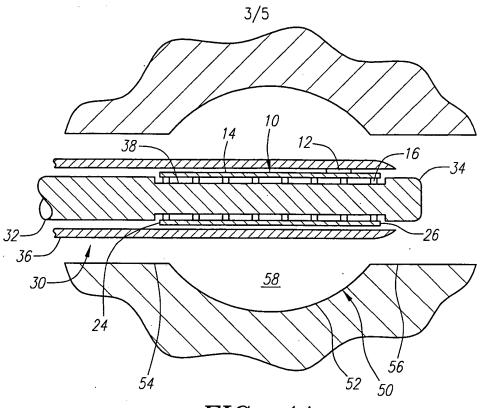


FIG. 4A

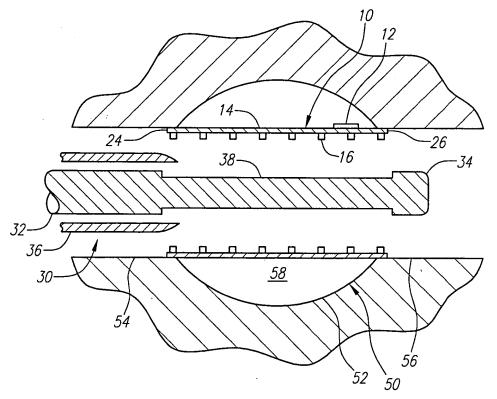


FIG. 4B



4/5

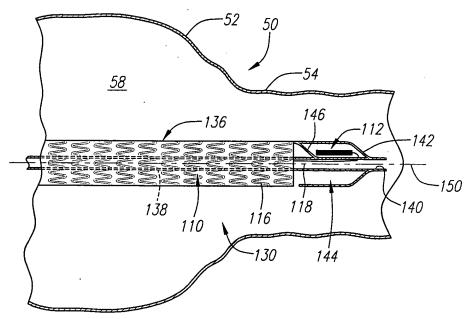


FIG. 5A

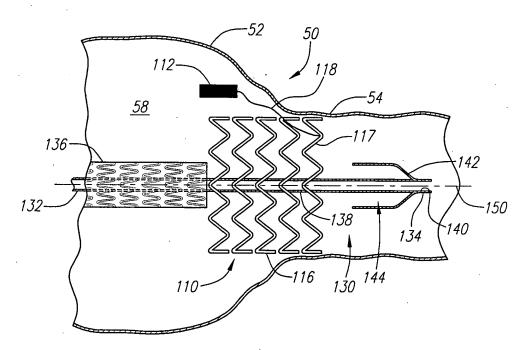


FIG. 5B



5/5

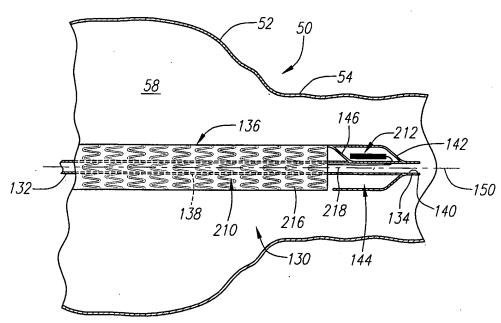


FIG. 6A

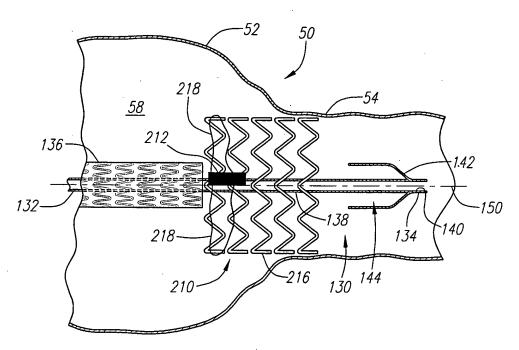


FIG. 6B